


Figure 1.

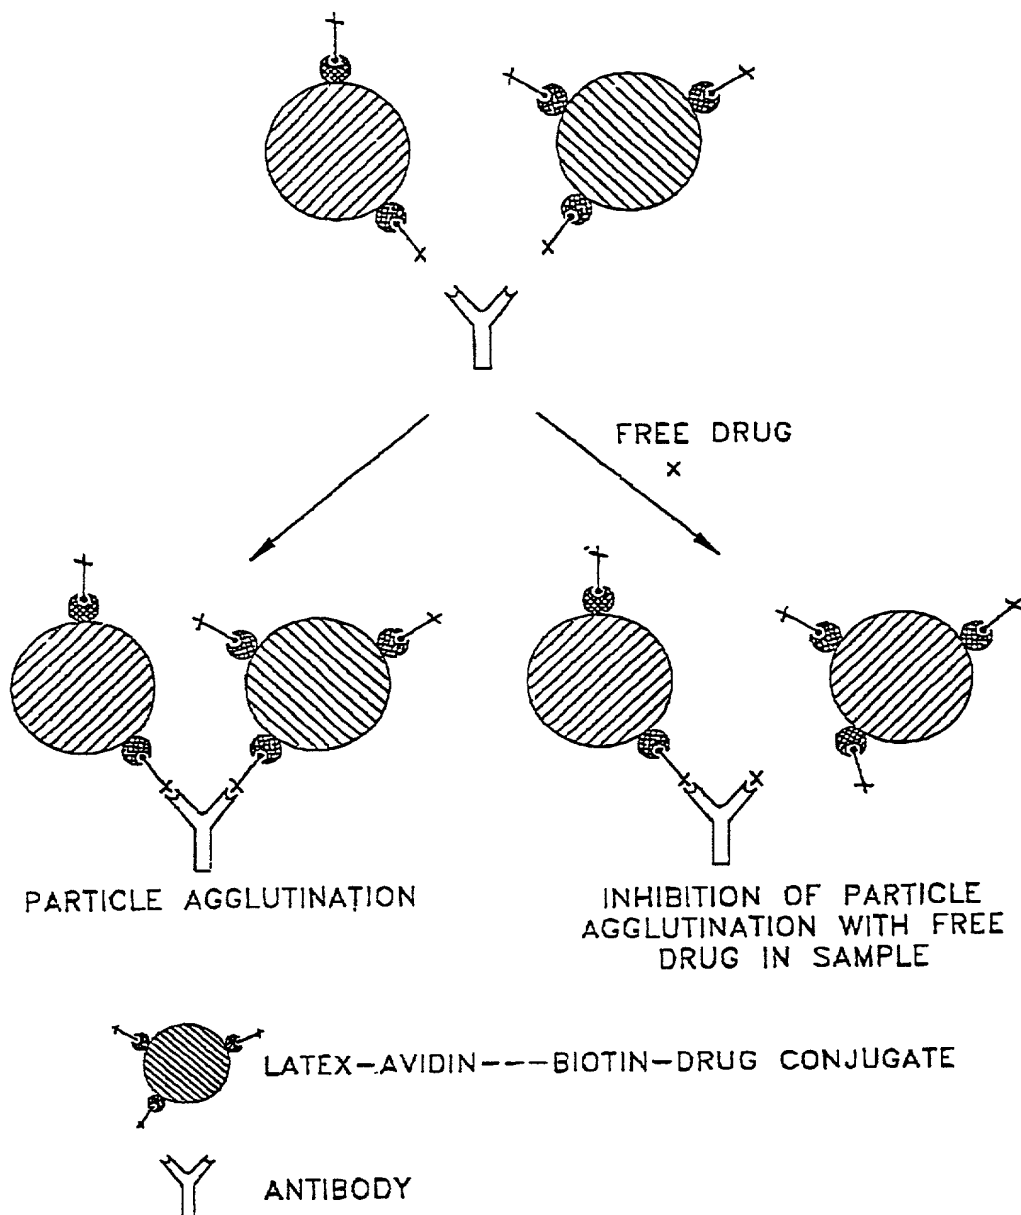

LATEX-BASED BIDENTATE IMMUNOINHIBITION ASSAY -
2-REAGENT SYSTEM

FIG. 2

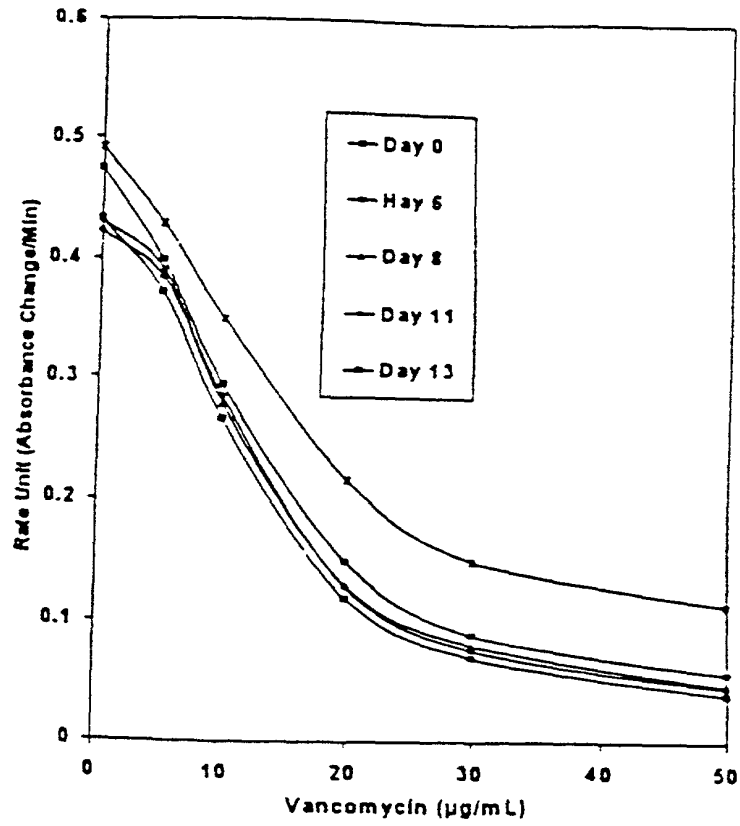


Figure 3

FO2250-50088860

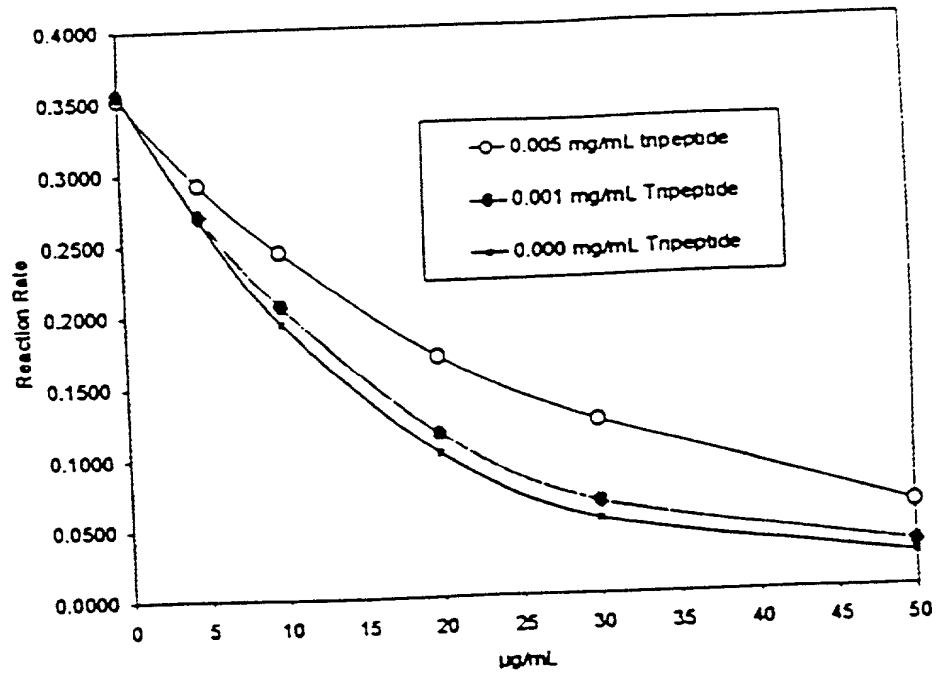


Figure 4

102290 50088860

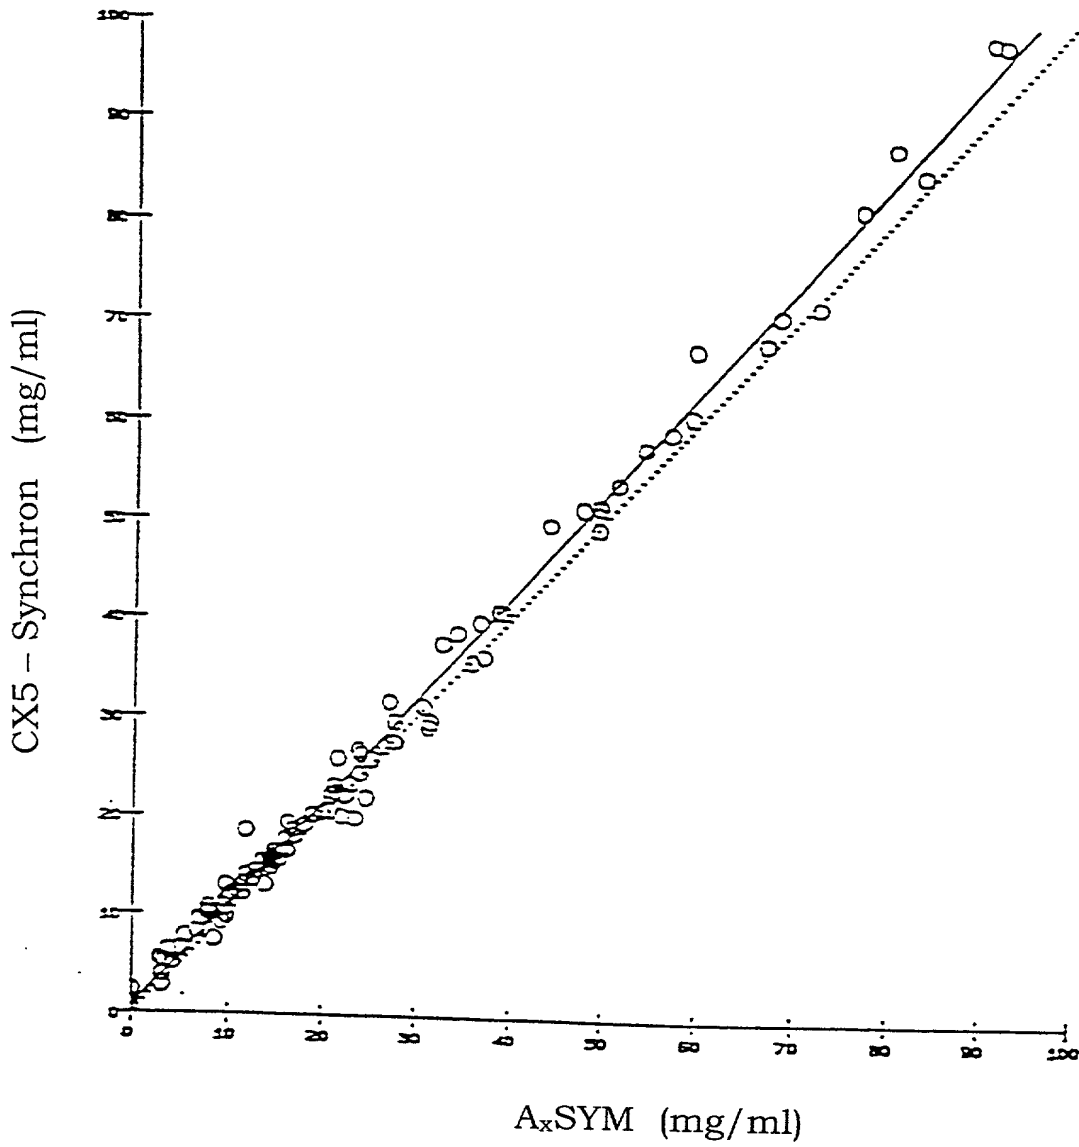


Figure 5

Fig. 6A

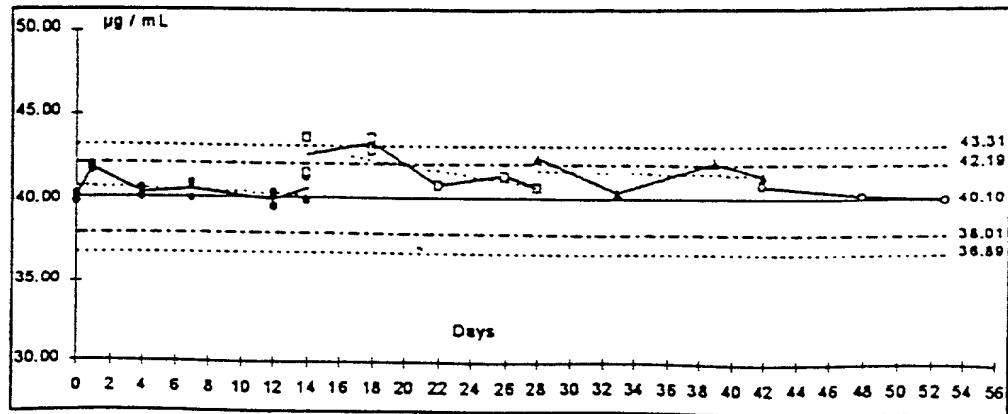


Fig. 6B

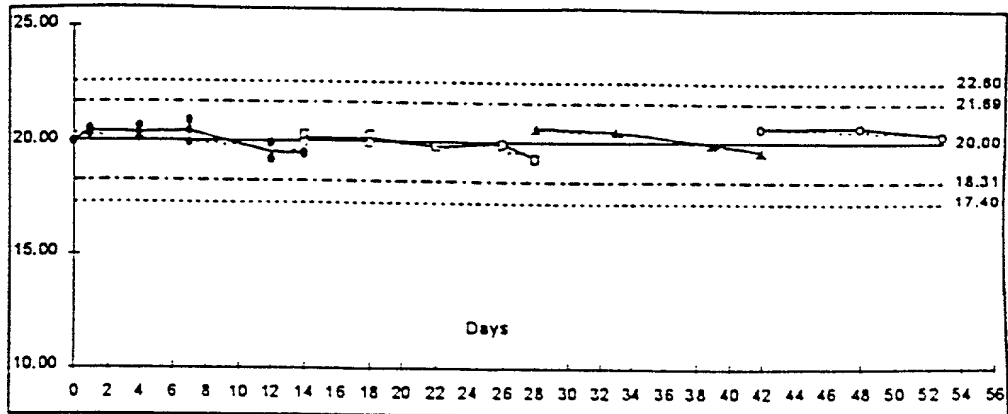


Fig. 6c

